

TITLE: IN-SITU INJECTION AND MATERIALS SCREENING DEVICE

APPLICANT: TREVOR FRANK et al.

DOCKET NO: 1012-076

1/12


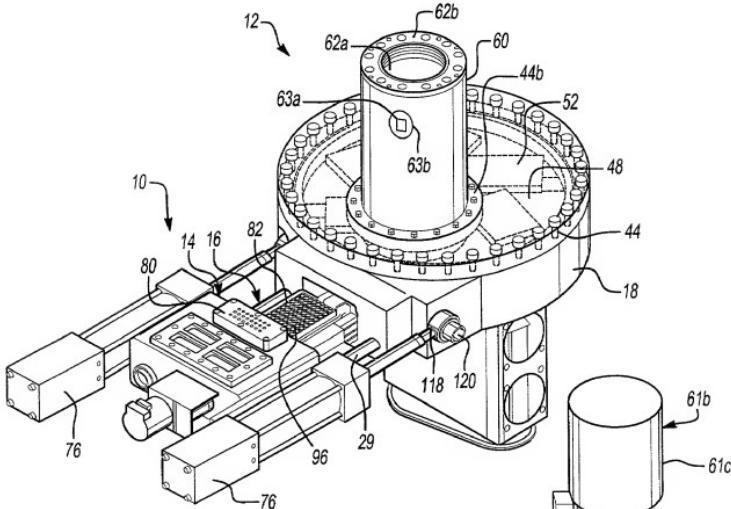


Fig-1

Fig-2

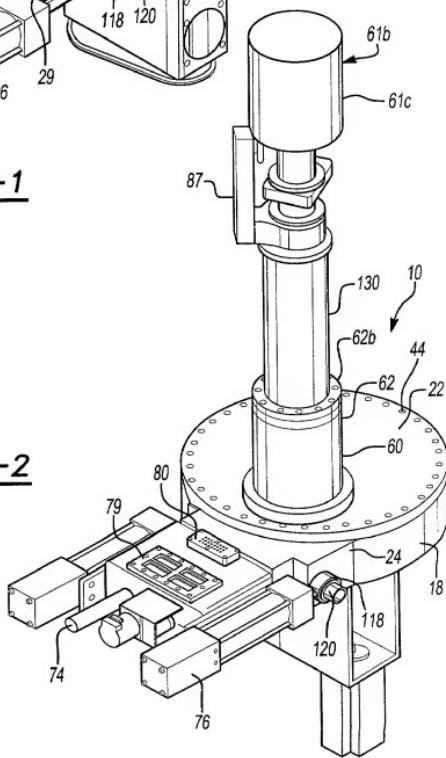

T06290 Sh656360

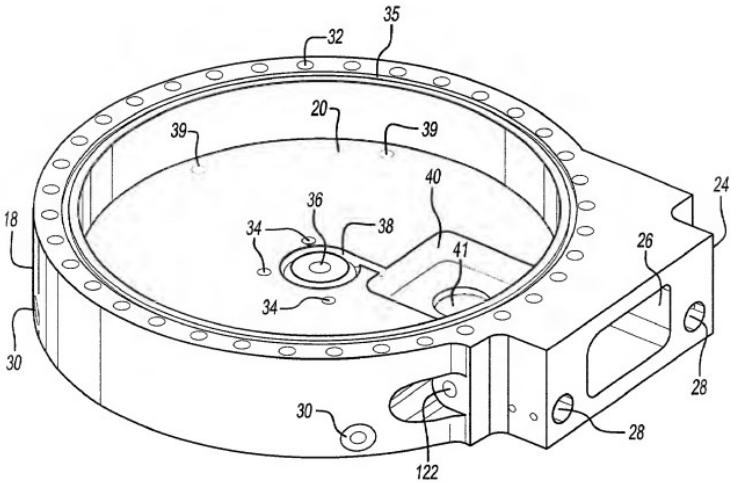


Fig-3a

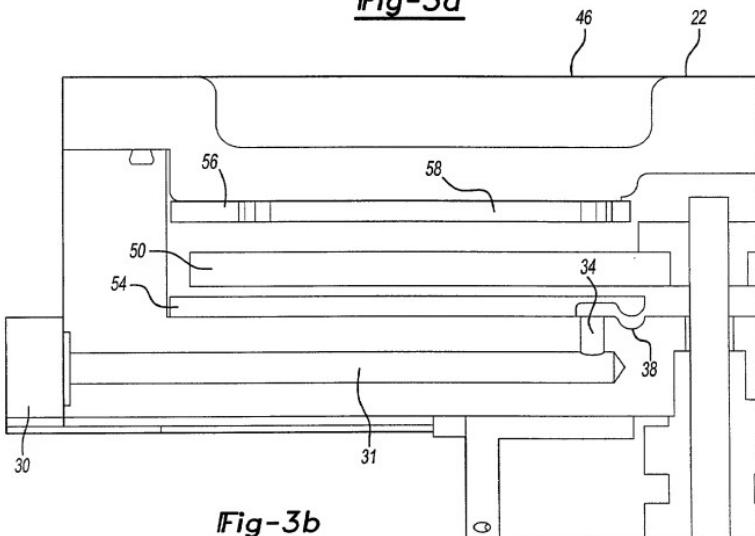


Fig-3b

TITLE: IN-SITU INJECTION AND MATERIALS SCREENING DEVICE

APPLICANT: TREVOR FRANK et al.

DOCKET NO: 1012-076

3/12

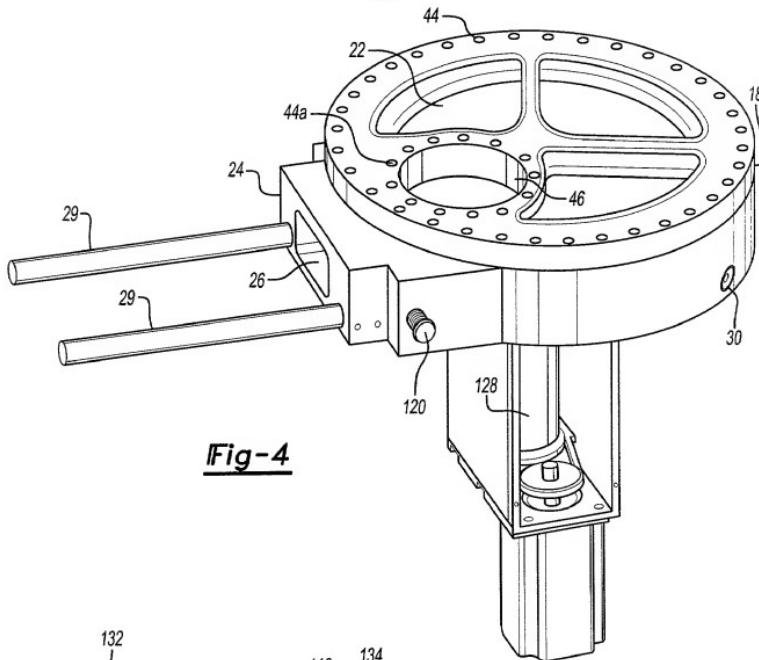


Fig-4

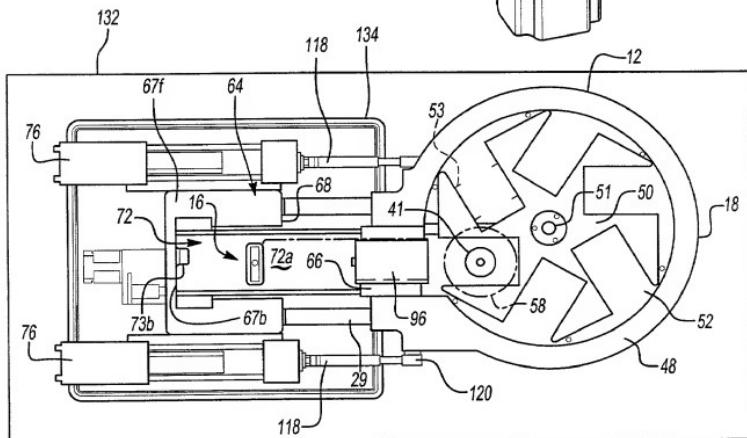


Fig-5a

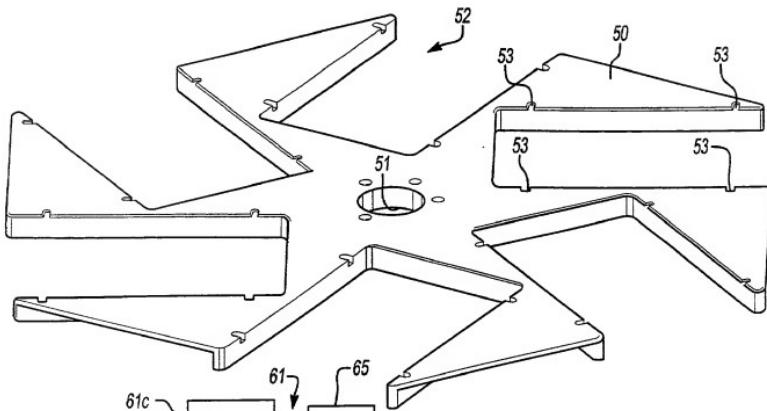


Fig-5b

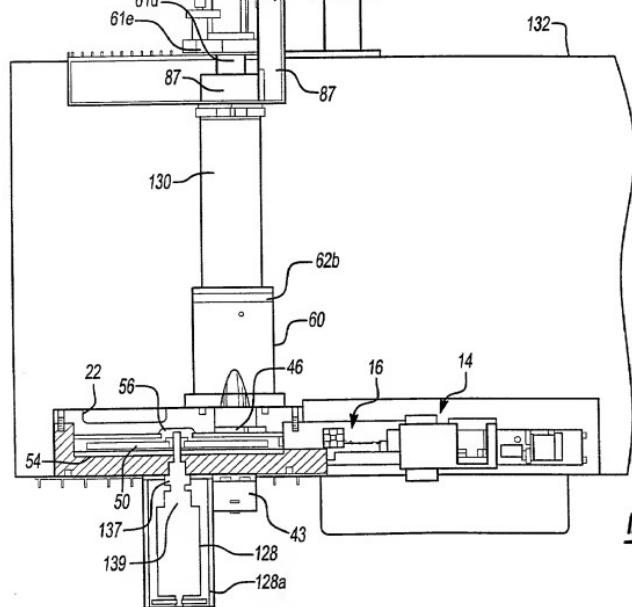


Fig-6

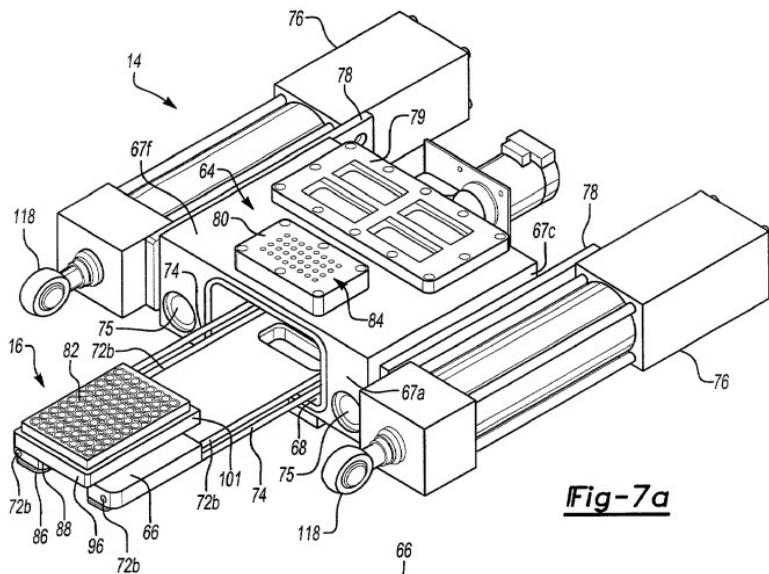


Fig-7a

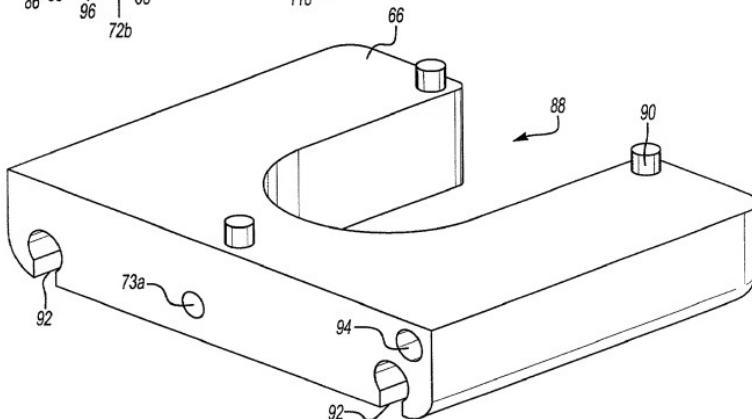


Fig-7b

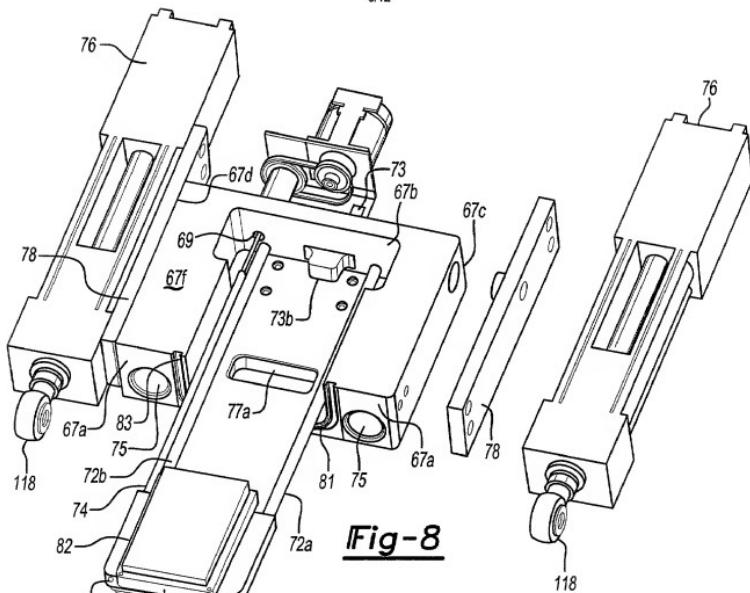


Fig-8

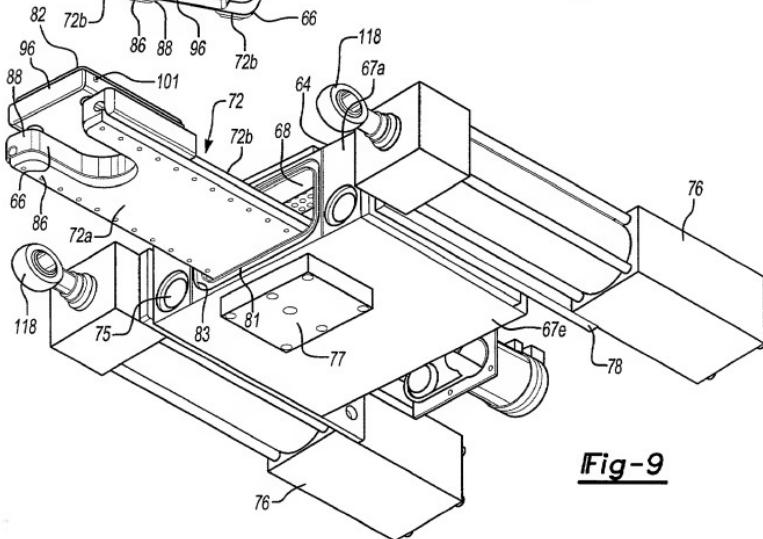


Fig-9

00063901-062001

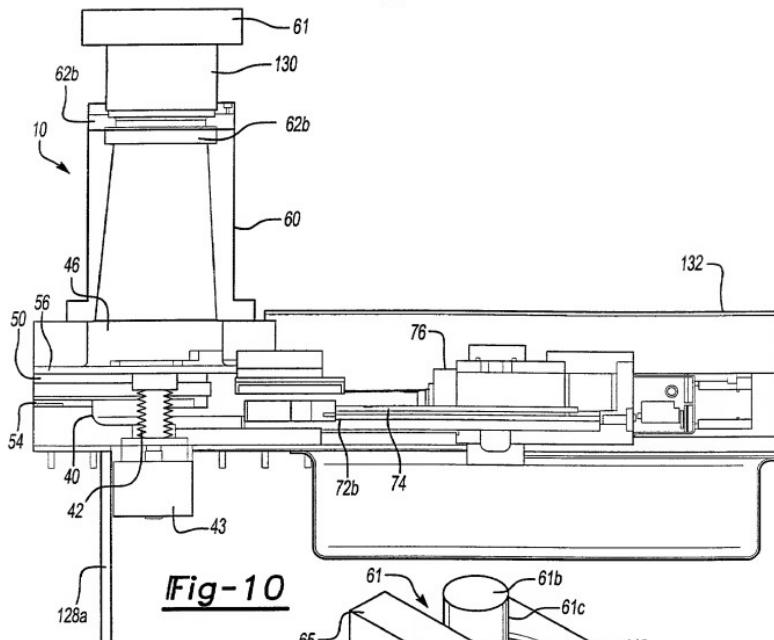


Fig-10

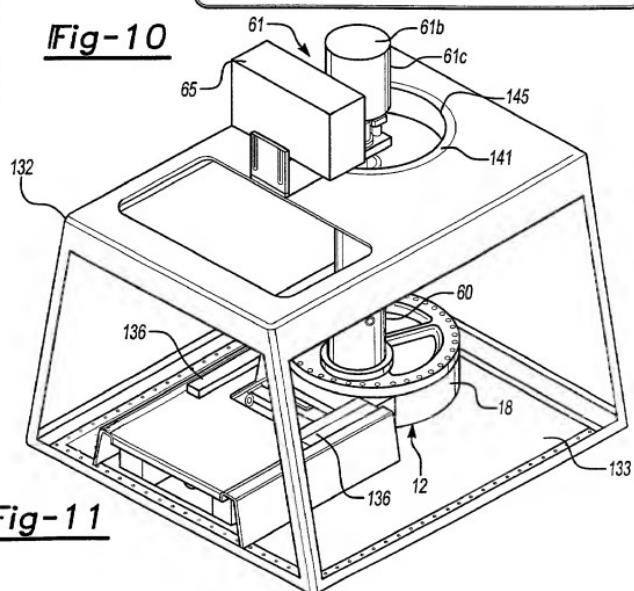


Fig-11

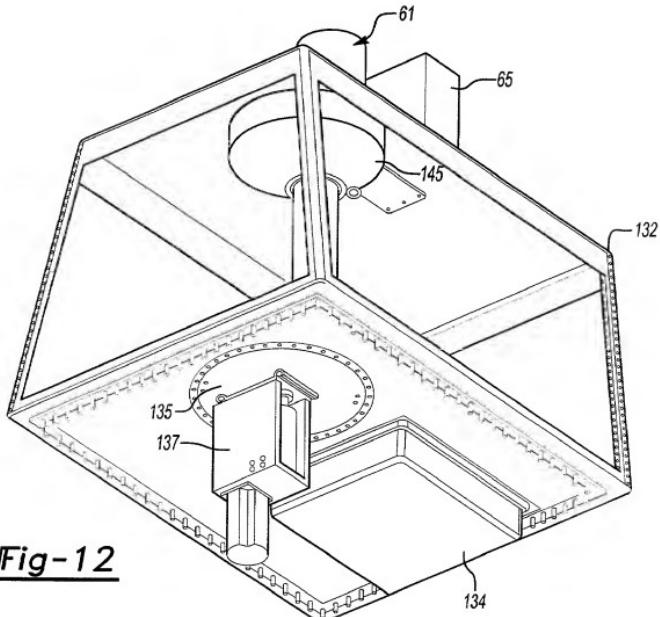


Fig-12

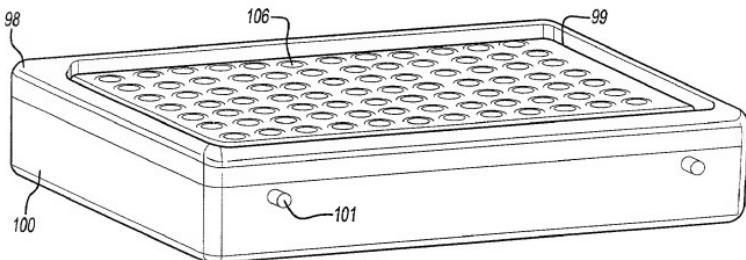


Fig-13

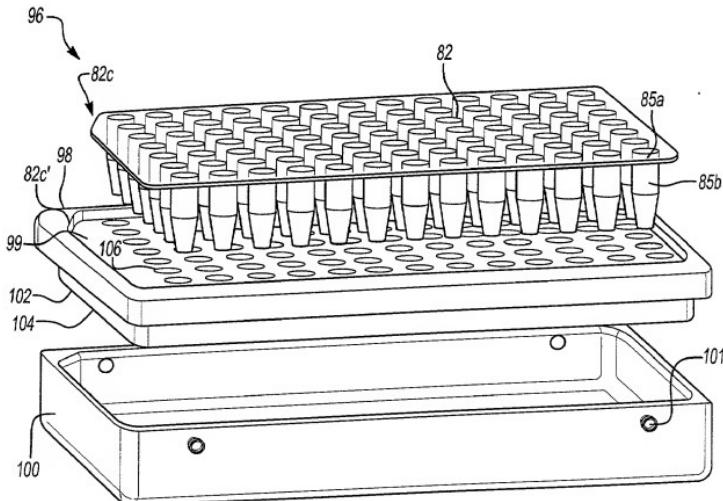


Fig-14

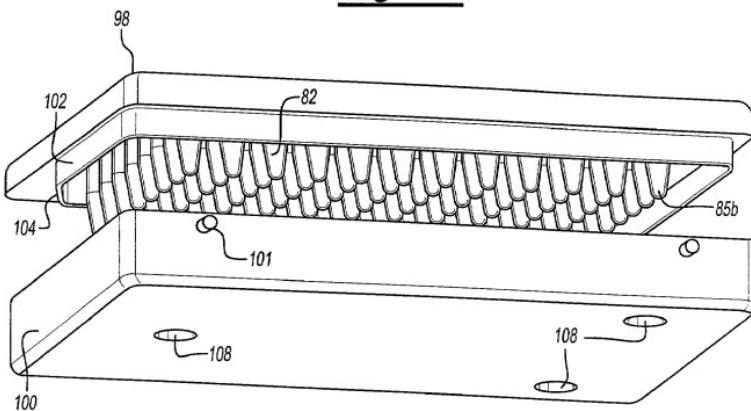


Fig-15

TITLE: IN-SITU INJECTION AND MATERIALS SCREENING DEVICE
APPLICANT: TREVOR FRANK et al.
DOCKET NO: 1012-076
10/12

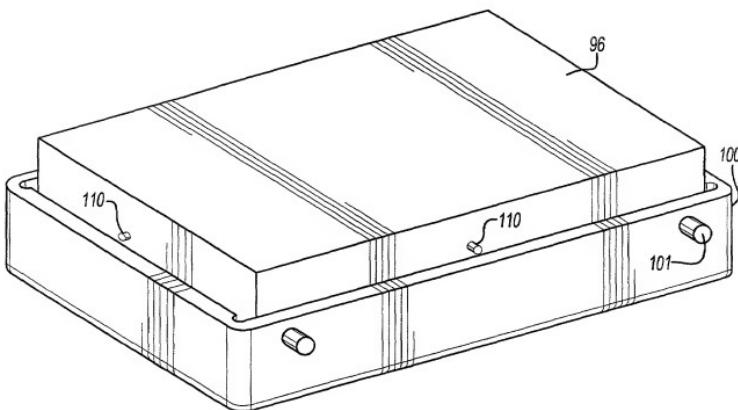


Fig-16


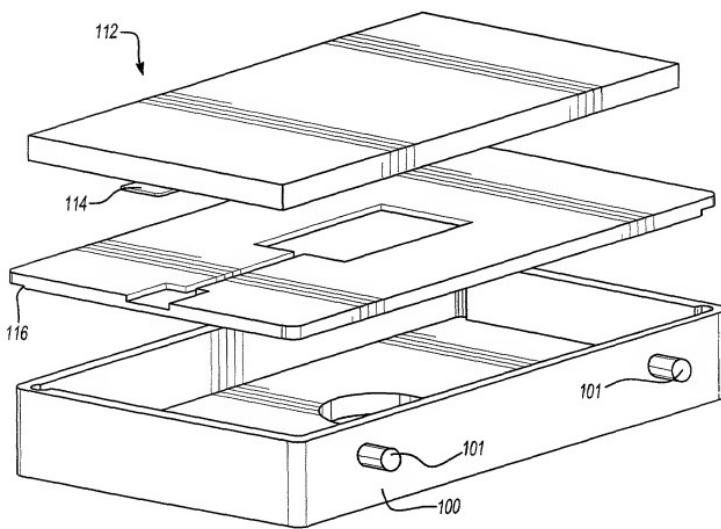


Fig-17



106290-Sh656860

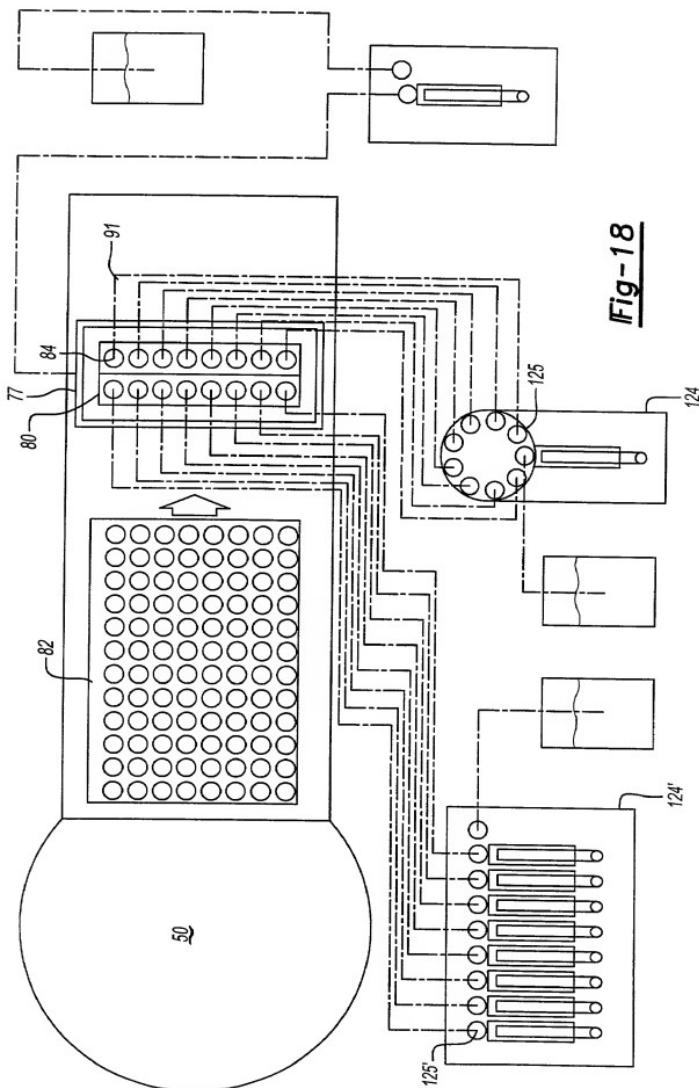